

# **Precision with Bite**






The resectoscopes from Richard Wolf



# Consistently efficient

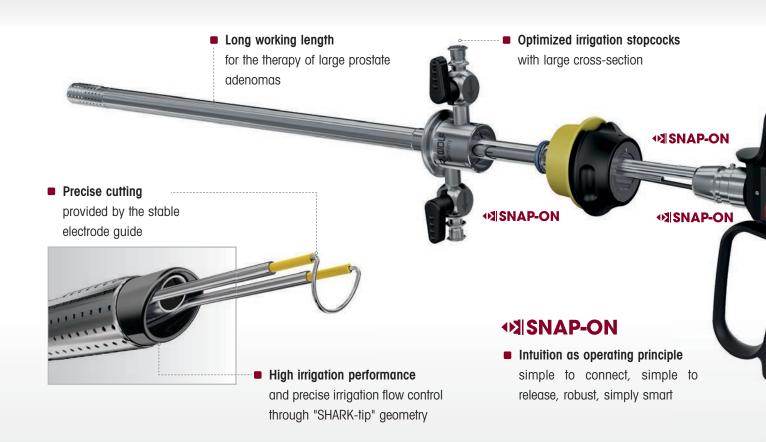

# Progress at every level.

Richard Wolf resectoscopes for urology have formed a platform for the therapeutic and diagnostic interventions at the highest level for many decades.

The **SHARK Resectoscope Line**, now takes quality, control and safety to a new dimension. **SHARK** combines years of global experience and user feedback with innovative technology. The result is a high-quality system with absolutely no compromises that makes your work more efficient. You are able to connect and disconnect the system elements with one simple action. Quick connection is combined with high stability. See for yourself!







# Ergonomic overall design Consistent ergonomically designed working elements for more efficiency and control

# Quality in your hands Stainless steel, ceramic, and biocompatible plastics guarantee maximum service life

#### Perfect shape for your work

This was also confirmed by the prestigious International Forum Design (iF). Our **SHARK Resectoscopes** were awarded the coveted iF Product Design Award 2013. Alongside quality of design, the assessment criteria also include finish, functionality and ergonomic styling.



Precision and ergonomic design



# Precision at the cutting edge: Newly designed sheath system



"SHARK-tip" The oblique sheath tip at the distal end made of black ceramic permits focused irrigation and prevents reflection of light  Freedom of choice
 Continuous irrigation sheaths and variety of intermittent sheaths

 Freedom of movement Double sheath system with 360° rotatable inner sheath  Freedom of connection
 Inner and outer sheaths connectable in any position

with central stopcock

Optimalum flow
 Optimized irrigation stopcock
 with large cross-section and
 "SHARK-tip" geometry for ideal
 flow characteristics



# All applications under control: Monopolar and bipolar working elements





active and passive working elements with open or closed handle design, for left-handed and right-handed users

#### Ergonomic design

with special "SHARK-fin" finger supports and enlarged thumb rings for comfort

- **Soft stop** for fatigue-free working
- Torsion-resistant connector for all system components

#### Twist-lock

for secure connection of telescope and working element.

 Automatic snap-on electrode locking for intuitive fixation of the electrode












New perspectives in detail











- Monopolar and bipolar versions
- Enhanced stability

   on the basis of the newly
   designed structure for the
   electrode fork
- Precise electrode guidance through working element and telescope
- Maximum diversity for every application
- Automatic snap-on elelctrode locking at the working element
- Color coding for simplified assignment of system components







Monopolar resectoscopes



#### Sheaths for intermittent irrigation



#### Monopolar working elements



Ds = Continuous irrigation

Direction of view

12°

30°

Sheath size

22/24 Fr.

24 Fr.

24/26 Fr.

26 Fr.

Ds

IS


Ds

iS


is = intermittent irrigation

\*not suitable for 22/24 Fr. double sheath system



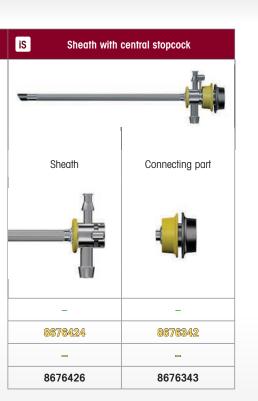

#### **Obturators**

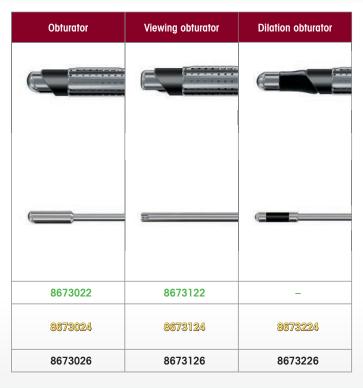

### Telescopes, Ø 4 mm





Monopolar electrodes

# 12°/30°, for multiple use, monopolar

				for sheath	sizes [in Fr.]		Colo	or code	<u> </u>
	Designation	Loop	Ds 22/24	<b>I</b> S 24	Ds 24/26	<b>iS</b> 26	Fork	Stem	Туре
			~	_	_	-	green	Dark gray	86782235
		Loop ø 0.35 mm	_	~	~	_	yellow	Dark gray	86782435
	Cutting		_	_	-	~	black	Dark gray	86782635
6	electrode	Loop ø 0.8 mm	_	V	r	_	yəllow	Dark gray	86782480
6	Coagulation		~	~	~	_	green	Dark gray	86782201
C.	electrode	Roller	_	-	-	<b>v</b>	black	Dark gray	86782601
	Coagulation electrode	Sphere	~	V	~	-	green	Dark gray	86782202
1	Coagulation	Button	~	~	~	_	green	Dark gray	86782203
	electrode	DUIIOIT	-	-	-	~	black	Dark gray	86782603
	Knife	Knife	~	~	~	-	green	Dark gray	86782204
-	electrode	Rille	_	-	-	~	black	Dark gray	86782604
	Hook	Hook	~	~	~	-	green	Dark gray	86782205
-	electrode	TIOOK	-	-	-	~	black	Dark gray	86782605
6	EVAP electrode	barrel-shaped	-	V	~	V	yellow	Dark gray	86782407
\$	EVAP electrode	Pyramid	_	V	~	V	yellow	Dark gray	86782408
-		Wing	<b>v</b>	-	_	-	green	Dark gray	86782206
6	EVAP electrode	(loop profile flat)	-	~	~	-	yəllow	Dark gray	86782406
		liui)	-	-	-	✓	black	Dark gray	86782606

✓ suitable for the relevant sheath size – not suitable

Ds = Continuous irrigation



# 0°, for multiple use, monopolar

	Baadan atlan			for sheath	sizes [in Fr.]		Color	code	<b>.</b>
	Designation	Loop	Ds 22/24	18 24	Ds 24/26	<b>iS</b> 26	Fork	Stem	Туре
	Cutting	Loop	_	~	~	_	yellow	Dark gray	86792435
0	electrode	ø 0.35 mm	_	_	_	~	black	Dark gray	86792635
5	Coagulation electrode	Roller	_	V	r	_	green	Dark gray	86792201
	Coagulation electrode	Sphere	_	V	v	~	iransparent	Dark gray	86792202
5	EVAP electrode	barrel-shaped	-	V	v	~	yellow	Dark gray	86792407
	Knife electrode	Knife	_	V	v	V	iransparent	Dark gray	86792204
-	Hook electrode	Hook	_	V	v	V	iransparent	Dark gray	86792205



Monopolar electrodes

# $12^{\circ}\!/30^{\circ}\!,$ for single use, sterile\*, monopolar

	Baatan attan			for sheath	sizes [in Fr.]		Colo	or code	Туре
	Designation	Loop	Ds 22/24	<b>I</b> S 24	Ds 24/26	<b>iS</b> 26	Fork	Stem	
			~	_	_	_	green	transparent	46782235
	Cutting	Loop ø 0.35 mm	_	~	~	_	yəllow	transparent	46782435
	electrode	<i>p</i>	-	-	-	~	black	transparent	46782635
	(pack of 10)	Loop	~	-	-	_	green	transparent	46782225
5		ø 0.25 mm	-	~	<b>v</b>	-	yellow	transparent	46782425
	Cutting electrode (pack of 5)	Loop ø 0.8 mm	_	V	r	_	yellow	transparent	46782480
	Hook		~	V	~	-	green	transparent	46782205
	electrode (pack of 5)		_	_	_	V	black	transparent	46782605
S.	Coagulation electrode (pack of 5)	Roller	~	۷	v	_	green	transparent	46782201
6	Coagulation electrode (pack of 5)	Sphere	~	۷	v	_	green	transparent	46782202
1	Coagulation	Dutter	~	~	~	_	green	transparent	46782203
	electrode (pack of 5)		_	_	_	V	black	transparent	46782603
-	Knife	1/ nife	~	V	~	_	green	transparent	46782204
	electrode (pack of 5)	electrode Knife pack of 5)	_	_	-	~	black	transparent	46782604

✓ suitable for the relevant sheath size

size – not suitable

is = intermittent irrigation

Ds = Continuous irrigation



# $0^\circ\text{, for single use, sterile*, monopolar}$

	Designation	Loon	for sheath sizes [in Fr.]				Color code		Ture
	Designation	Designation Loop	Ds 22/24	<b>i</b> S 24	Ds 24/26	<b>iS</b> 26	Fork	Stem	Туре
	Cutting	Loop	_	v	V	_	yəllow	transparent	46792435
0	electrode (pack of 5)	ø 0.35 mm	_	_	-	V	black	transparent	4679263
	Hook electrode (pack of 5)	Hook	_	V	v	_	transparent	transparent	4679220
5	Coagulation electrode (pack of 5)	Roller	_	v	V	_	green	transparent	4679220
	Knife electrode (pack of 5)	Knife	_	v	v	_	transparent	transparent	4679220

✓ suitable for the relevant sheath size - not suitable \* packed single, sterile

Ds = Continuous irrigation is = intermittent irrigation

\_

# HF connection cable, monopolar

Connection of HF device	Manufacturer of HF device	Length	Туре
		3 m	815.032
	ERBE, ACC, ICC	5 m	815.052
	EDDE T Carias	3 m	815.132
	ERBE T Series	5 m	815.152
	Martin Develted Accounter	3 m	815.031
	Martin, Berchtold, Aesculap	5 m	815.051
~	Davia Vallavlah Esha lat	3 m	815.033
	Bovie, Valleylab, Erbe Int.	5 m	815.053
	Eschmann	3 m	815.034
	and other devices with a 4 mm plug	5 m	815.054




Bipolar resectoscopes



#### Sheaths for intermittent irrigation



#### **Bipolar working elements**

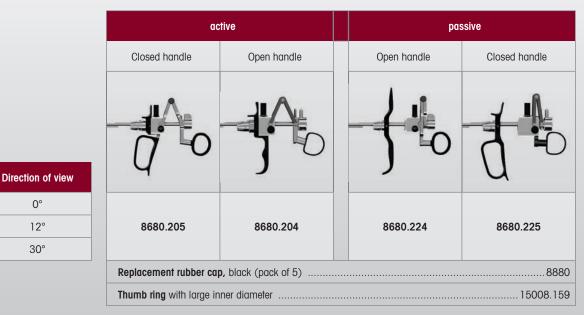

Ds = Continuous irrigation

Sheath size

22/24 Fr.

24 Fr.

24/26 Fr.

26 Fr.


Ds

IS

Ds

iS



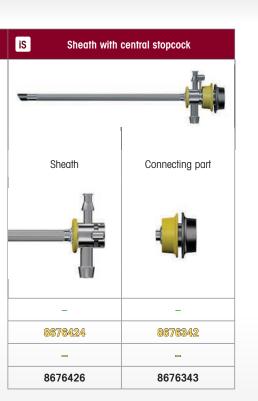

#### **Obturators**



### Telescopes, Ø 4 mm





Bipolar electrodes

# 12°/30°, for multiple use, bipolar

	Designation	Loop	for sheath sizes [in Fr.]				Color code		Tuno
	Designation	гоор	Ds 22/24	<mark>1</mark> 8 24	Ds 24/26	<b>iS</b> 26	Fork	Stem	Туре
	Cutting	Loop	~	_	-	-	blue	<b>yello</b> w	8622133
5	electrode	ø 0.3 mm	_	~	v	v	blue	<b>yello</b> w	8622131
	Coagulation electrode	Cylinder ø 1.2 mm	v	v	v	v	blue	yəllow	8623022
	Hook electrode	Hook	r	V	v	v	blue	yəllow	862309

✓ suitable for the relevant sheath size – not suitable

Ds = Continuous irrigation



# $0^\circ\!,$ for multiple use, bipolar

	Decimation	Loon		for sheath s	sizes [in Fr.]	Color code		Turne	
	Designation	Loop	Ds 22/24	18 24	Ds 24/26	<b>is</b> 26	Fork	Stem	Туре
6	Cutting electrode	Loop ø 0.3 mm	_	V	V	_	blue	yəllow	8609031



Bipolar electrodes

# $12^{\circ}/30^{\circ}$ , for single use, sterile\*, bipolar

	Besternetten	1		for sheath	sizes [in Fr.]		Color	code	Туре
	Designation	Loop	Ds 22/24	<mark>1</mark> 8 24	DS 24/26	<b>iS</b> 26	Fork	Stem	
			~	-	-	-	blue	blue	4622.1333
	Cutting	Loop ø 0.3 mm	_	~	~	_	blue	blue	4622.1313
	electrode	<i>p</i> 010 11111	_	_	-	<b>v</b>	green	blue	4624.1313
5	(pack of 3)	Loop	<b>v</b>	_	-	_	blue	blue	4622.2533
		ø 0.25 mm	-	~	~	~	blue	blue	4622.2513
6	Cutting electrode, oval (pack of 3)	Loop ø 0.3 mm	_	~	~	V	blue	blue	4622.1323
	Coagulation electrode	Cylinder	~	_	_	_	blue	blue	4623.0243
5	(pack of 3)	ø Í.2 mm	_	~	~	V	blue	blue	4623.0223
	BiVAP electrode (pack of 3)	Donut	~	_	_	_	blue	blue	46300223
-			_	~	~	V	blue	blue	46300243

✓ suitable for the relevant sheath size - not suitable \* packed single, sterile

Ds = Continuous irrigation



# $0^\circ,$ for single use, sterile\*, bipolar

	Desimution	1	for sheath sizes [in Fr.]			Color code		Time	
	Designation	Loop	Ds 22/24	<b>IS</b> 24	Ds 24/26	<b>iS</b> 26	Fork	Stem	Туре
		Loop	_	~	~	-	blue	blue	4609.0313
	Cutting electrode	ø 0.3 mm	_	_	-	<b>v</b>	green	blue	4611.0313
electrode (pack of 3)		Loop ø 0.25 mm	_	V	~	_	blue	blue	4609.2513
	Cutting electrode, oval (pack of 3)	Loop ø 0.3 mm	_	v	~	v	blue	blue	4609.032
	Coagulation electrode (pack of 3)	Cylinder ø 1.2 mm	_	v	v	V	blue	blue	4610.0223
	BiVAP electrode (pack of 3)	Donut	_	V	~	v	blue	blue	46310243

✓ suitable for the relevant sheath size - not suitable \* packed single, sterile

Ds = Continuous irrigation

is = intermittent irrigation

# HF connection cable, bipolar

Connection of HF device	Manufacturer of HF device	Length	Туре
		3 m	8108.232
	ERBE	5 m	8108.252
	Marilla	3 m	8108.231
	Martin	5 m	8108.251



www.richard-wolf.com